


NEU

Nanofiber Electrospinning Unit




Development history

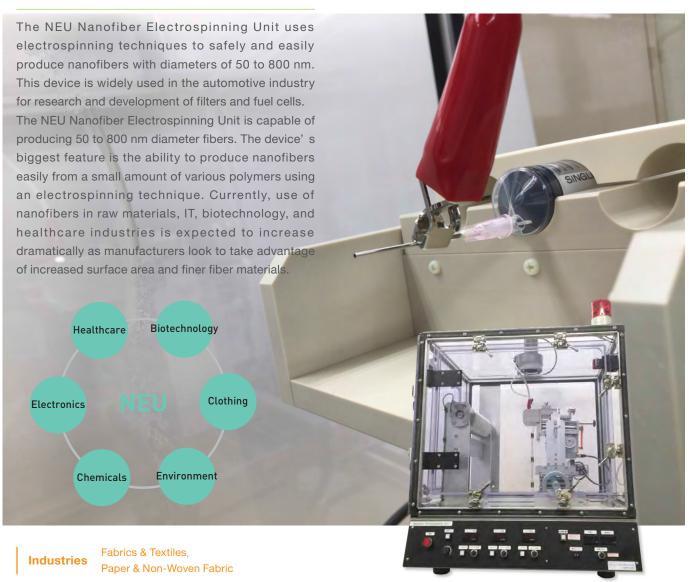

Despite active studies into electrospinning, only handmade devices were available. Although researchers at Drexel University attempted to manufacture a lab prototype, no company capable of producing a device with high accuracy could be found in the U.S. However, Kato Tech Co., Ltd. in Japan undertook the development of an electrospinning device for lab use and created a system that comprised a voltage generator and nozzle, rotating collector, a quantitative syringe pump, and a exhaust fan. This device largely featured the ideas of Drexel University's Dr. Frank Ko, a leading authority on electrospinning, and made it possible to create nanofibers easily by electrospinning.

Nano-fiber manufacturing principle

As shown in the diagram, the electrospinning device consists of a pointed positive electrode (capillary) and a flat negative (ground) electrode. High voltage is applied between the two electrodes, and the charged molten polymer or polymer solution coming from the capillary is attracted through the electric field toward the negative electrode. At this point, polymers with low molecular cohesion become a spray, and those with high molecular cohesion are further separated into fibers that are attracted to the negative electrode, where they form a thin layer of fibers.

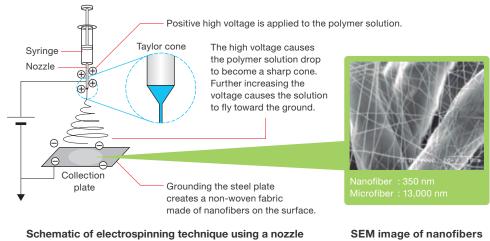

(conventional nozzle method)

NEU Nanofiber Electrospinning Unit

Dimensions/Weight (approx.)	$W900 \times D750 \times H1080 \ (mm) \ / \ 120 \ kg$ *Including pilot lamp
Power source	100 VAC, power consumption: 80W Max. *Ensure grounding
Measurement environment temperature and humidity	10 to 40°C / 30 to 70% RH (No condensation.)
High-voltage DC power	Voltage: 0 to 39 kV (displayed on digital meter) Leakage current: Max. 500 µA (displayed on digital meter)
Exhaust fan	Sirocco fan
Syringe pump	
Capacity	20 ml (standard)
Pieces	Up to 3 pcs.
Discharge speed	0.000 to 0.500 mm/min (Stable motor range: 0.030 mm to 0.250 mm/min) *When used with the 20 ml syringe
Traverse speed	0 to 300 mm/min

Distance between target and syringe	0 to 200 mm (with standard syringe and needle attached)
Unit adjustment angle	45° from the horizontal
Syringe height adjustment range	150 mm

Target

Drum type (standard)	Dimensions: 100 mm (diameter), 330 mm (width) Peripheral velocity: 0 to 9.00 m/min
	Drum type (standard)

Safety precautions

Standard	Spark limiter (stopping at 500 μA or higher) Door interlock	



For safety use, please read the operation manual / the instruction carefully and throughly before using the tester.

Specification details recorded here are subject to change without notice. We appreciate your understanding.



KATO TECH co.,LTD. http://english.keskato.co.jp/

Headquarters and Factory:

26 Karato-cho, Nishikujo, Minami-ku, Kyoto 601-8447, Japan TEL. +81-75-681-5244 (main), +81-75-693-1660 (sales dept.) FAX. +81-75-681-5243 E-mail. katotech@keskato.co.jp

Shanghai Office: Kato Tech Shanghai Representative Office

UnitA7, 14/F Huafu Mansion, 585LongHuaRD, W. shanghai 200232, China TEL. +86-(0)21-5836-2290 FAX. +86-(0)21-6469-1121

E-mail. shanghai@keskato.co.jp